


F16. 1

All or

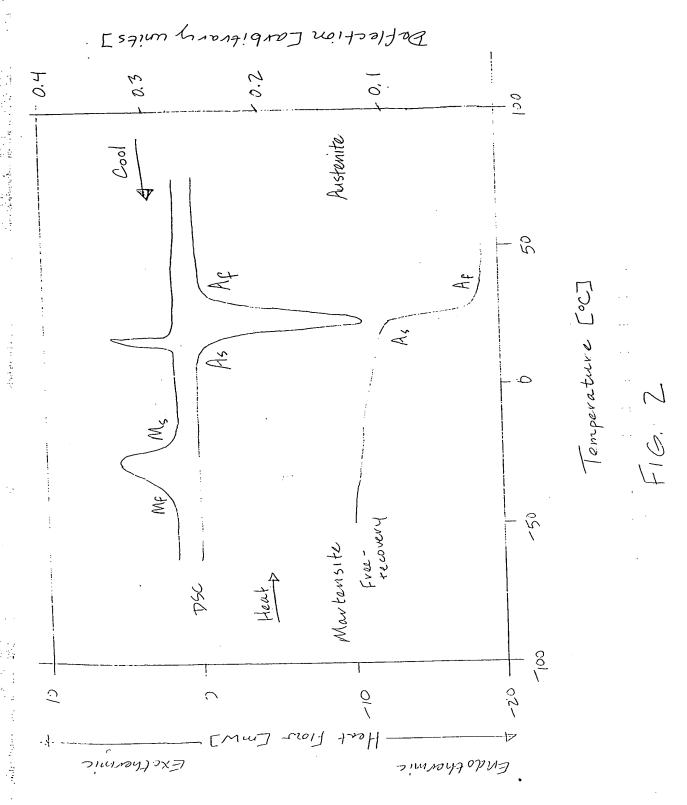



AVOIDING STRESS-INDUCED MARTENSITIC TRANSFORMATION IN MEDICAL DEVICES


SERIAL NO.: TBD; ENDOV-55675

SERIAL NO.: TBD; ENDOV-55675

SERIAL NO.: TBD; ENDOV-55675

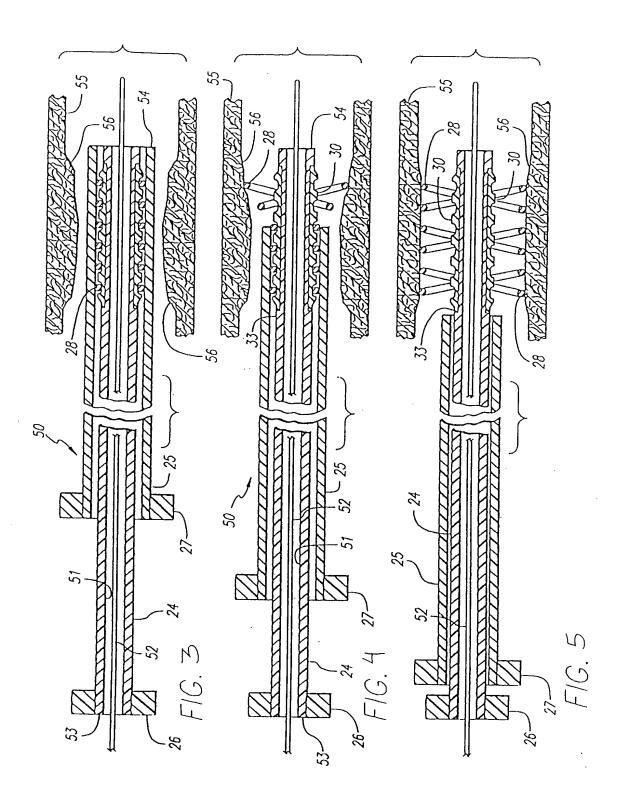

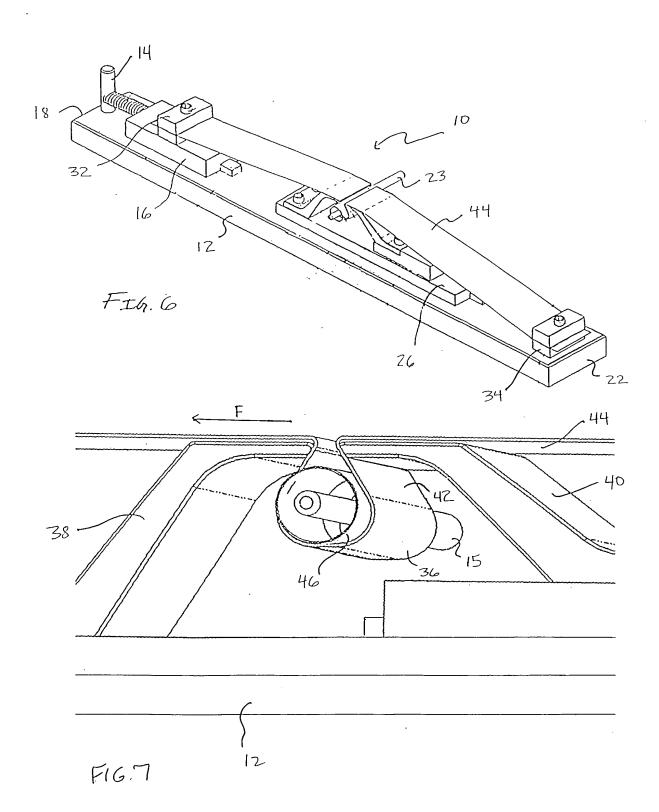

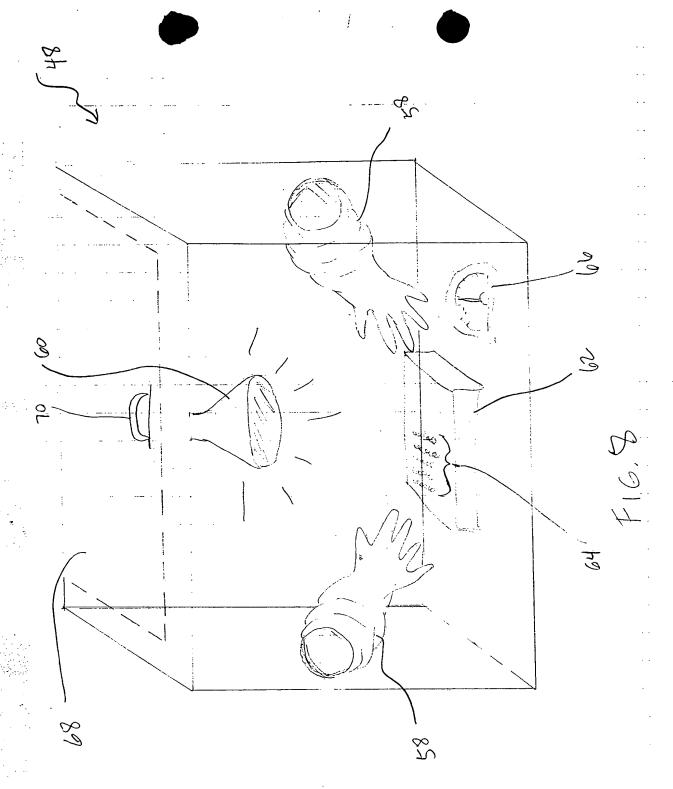

AVOIDING STRESS-INDUCED MARTENSITIC TRANSFORMATION IN SERIAL NO.: TBD; ENDOV-55675

SERIAL NO.: TBD; ENDOV-55675

